

National Institute of Neurological Disorders and Stroke  
Biorepository:

**BioSpecimen Exchange for Neurological Disorders, BioSEND**

Biospecimen Collection, Processing, and Shipment Manual for  
The role of **Microglia In Parkinson's disease Cognitive and  
MotoR Impairment +PD (MICRO-PD)**

## Table of Contents

<b>1.0</b>	<b><a href="#">Purpose</a></b> .....	<b>4</b>
<b>2.0</b>	<b><a href="#">Abbreviations</a></b> .....	<b>4</b>
<b>3.0</b>	<b><a href="#">BioSEND Information</a></b> .....	<b>5</b>
3.1	<a href="#">BioSEND Contacts</a>	
3.2	<a href="#">Hours of Operation</a>	
3.3	<a href="#">Holiday Schedules</a>	
3.4	<a href="#">Holiday Observations</a>	
<b>4.0</b>	<b><a href="#">BioSEND Sample Requirements</a></b> .....	<b>7</b>
4.1	<a href="#">Protocol Schedule for Biospecimen Submission</a>	
<b>5.0</b>	<b><a href="#">Specimen Collection Kits, Shipping and Supplies</a></b> .....	<b>9</b>
5.1	<a href="#">Kit Supply to Study Sites</a>	
5.2	<a href="#">Specimen Collection Kit General Contents</a>	
5.3	<a href="#">Specimen Collection Kit Contents</a>	
5.4	<a href="#">Site Required Equipment</a>	
<b>6.0</b>	<b><a href="#">Specimen Labels</a></b> .....	<b>12</b>
6.1	<a href="#">Types of Labels</a>	
6.2	<a href="#">Affixing Labels</a>	
<b>7.0</b>	<b><a href="#">Specimen Collection and Processing Procedures</a></b> .....	<b>14</b>
7.1	<a href="#">Blood Collection Protocols</a>	
7.2	<a href="#">Filling Aliquot Tubes</a>	
<b>8.0</b>	<b><a href="#">Packaging and Shipping Instructions</a></b> .....	<b>16</b>
8.1	<a href="#">Specimen Collection and Processing Form</a>	
8.2	<a href="#">Shipping Instructions</a>	
8.3	<a href="#">Shipping Address</a>	
<b>9.0</b>	<b><a href="#">Reconciliation and Non-Conformance</a></b> .....	<b>18</b>
<b>10.0</b>	<b><a href="#">Appendices</a></b> .....	<b>19</b>

- Appendix B: Whole Blood Collection for Isolation of Plasma and Buffy Coat
- Appendix D: Whole Blood Collection (No Processing)
- Appendix F: Whole Blood Collection for the Isolation of Serum
- Appendix I: Specimen Collection and Processing Form
- Appendix K: Frozen Shipping Instructions
- Appendix Q: UPS ShipExec™ Thin Client Instructions

## 1.0 PURPOSE

The purpose of this manual is to provide collection site staff (PIs, study coordinators, and the sample collection and processing teams) at various study sites with instructions for collection and submission of biological samples. It includes instructions for biospecimen submission to the BioSpecimen Exchange for Neurological Disorders (BioSEND) located at Indiana University.

This manual includes instructions for the collection, processing, aliquoting and shipping of the following samples:

- Serum
- Plasma
- Buffy Coat (for DNA extraction)
- Whole Blood
- PBMC

These procedures are relevant to all study personnel responsible for processing blood specimens to be submitted to BioSEND.

## 2.0 ABBREVIATIONS

BioSEND	BioSpecimen Exchange for Neurological Disorders
EDTA	Ethylene Diamine Tetra-acetic Acid
IATA	International Air Transport Association
PDBP	Parkinson's Disease Biomarkers Program
RBC	Red Blood Cells
RCF	Relative Centrifugal Force
RPM	Revolutions Per Minute

## 3.0 BioSEND INFORMATION

### 3.1 BioSEND Contacts

**Tatiana Foroud, PhD, Principal Investigator**

**Claire Wegel, MPH, Project Manager**

Email: [cwegel@iu.edu](mailto:cwegel@iu.edu)

**Ashley Garwood, CCRP, Clinical Research Coordinator**

Email: [hoviousa@iu.edu](mailto:hoviousa@iu.edu)

#### **General BioSEND Contact Information**

Phone: 317-278-6158

Email: [biosend@iu.edu](mailto:biosend@iu.edu)

Website: [www.BioSEND.org](http://www.BioSEND.org)

#### **Sample Shipment Mailing Address**

BioSEND

Indiana University School of Medicine

351 W. 10<sup>th</sup> Street, TK-217

Indianapolis, IN 46202-4118

### 3.2 Hours of Operation

Indiana University business hours are from 8 AM to 5 PM Eastern Time, Monday through Friday.

**Frozen samples must be shipped Monday- Wednesday only.**

For packaging and shipment details, please refer to Appendix K (Frozen Shipping Instructions)

Check the weather reports and the shipping courier website to make sure impending weather events (blizzards, hurricanes, etc.) will not impact the shipping or delivery of the samples. Couriers often reports anticipated weather delays on their website.

### 3.3 Holiday Schedules

- Please note that courier services may observe a different set of holidays. Please be sure to verify shipping dates with your courier prior to any holiday.
- **Weekend/holiday deliveries will not be accepted.**

### 3.4 Holiday Observations

Date	Holiday
January 1	New Year's Day
3 <sup>rd</sup> Monday in January	Martin Luther King, Jr Day
4 <sup>th</sup> Monday in May	Memorial Day
June 19	Juneteenth (observed)
July 4	Independence Day (observed)
1 <sup>st</sup> Monday in September	Labor Day
4 <sup>th</sup> Thursday in November	Thanksgiving
4 <sup>th</sup> Friday in November	Friday after Thanksgiving
December 25	Christmas Day

Please note that BioSEND has extended closures to inbound shipments around the Thanksgiving and Christmas holidays. In addition to sending advance notification of these closures to sites, dates will be posted on the BioSEND website. Frozen specimens collected during this period should be held at your site to ship after the first business day in January. If you are ever unsure if it is safe to ship samples, please email [biosend@iu.edu](mailto:biosend@iu.edu) to confirm.

For up-to-date holiday closure information and instructions, please visit <https://biosend.org/holiday-closures>.

## **4.0 BIOSEND SAMPLE REQUIREMENTS**

NINDS approves each study for a specific biospecimen collection protocol. Studies and study sites should make every effort to meet their approved biospecimen collection requirements.

If a sample is not obtained at a particular visit, this should be recorded in the notes section of the Sample Collection and Processing Form. This form should be submitted to BioSEND on or prior to the date of shipment. A physical copy should also be included in the sample shipment to BioSEND.

Note: All samples in this protocol will ship frozen on dry ice to BioSEND

**4.1 Protocol Schedule for Biospecimen Submission to BioSEND – MICRO-PD**

<b>Visit (month)</b>	<b>BL</b>
Serum aliquots, 1.5ml	3
Plasma aliquots, 1.5ml	3
Buffy Coat	1
Whole Blood, 3ml	1
PBMC aliquot, 5ml	2



## 5.0 SPECIMEN COLLECTION KITS, SHIPPING KITS AND SUPPLIES

BioSEND will provide labels and supplies only for those specimens that are to be shipped back to the BioSEND repository. Any tubes that will remain at the collection site or shipped to other repositories should be labeled accordingly. Links to each study's kit request module, sample submission forms, and other information can be found at <https://biosend.org/coordinate-studies/active-studies>

### 5.1 Ordering Kits and Supplies

Study sites are responsible for ordering study kits. We advise sites to proactively confirm kits are on hand ahead of study visits.

Kits and individual items can be ordered as required through the BioSEND kit request module:

- **MICRO-PD:** <https://redcap.link/MICRO-PD>

Please allow **TWO weeks** for kit orders to be processed and delivered.

**5.2 Specimen Collection Kit Contents**

Collection kits contain the following (for each subject) as designated per your protocol and/or NINDS resource development agreement. Do not replace or supplement any of the tubes or kit components provided with your own supplies unless you have received approval from the NINDS/BioSEND Study team to do so. Please store all kits at room temperature until use

<b>MICRO-PD Blood Collection Kit</b>	
<b>Supply</b>	<b>Quantity</b>
Cryovial (Sarstedt®) with purple cap, 2ml	19
Cryovial (Sarstedt®) with clear cap, 2ml	5
Cryovial (Sarstedt®) with red cap, 2ml	17
EDTA (glass) tube, 10ml	3
Serum (glass) tube, 10ml	2
EDTA (plastic) tube, 3ml	2
PBMC tube, 10ml	5
Bubble-tube sleeve	12
Cryobox, 25 cell	1
Disposable pipet, 3ml	2
Internal labels	50
Label set (kit & specimen labels)	1
Plastic Biohazard bag with absorbent sheet	2

<b>MICRO-PD Standard Shipping Kit</b>	
<b>Supply</b>	<b>Quantity</b>
Shipping box/ Styrofoam container	1
UN3373 Category B Label	1
Fragile Label	1
Dry Ice Label	1
UPS Airbill Sleeve	1

<b>MICRO-PD Bulk Shipping Kit</b>	
<b>Supply</b>	<b>Quantity</b>
Large shipping box/ Styrofoam container	1
UN3373 Category B Label	1
Fragile Label	1
Dry Ice Label	1
UPS Airbill Sleeve	1

## 5.4 Site Required Equipment

The following materials and equipment are necessary for the processing of specimens at the collection site and are to be **supplied by the local site**:

- Personal Protective Equipment: lab coat, nitrile/latex gloves, safety glasses
- Tourniquets
- Alcohol Prep Pads
- Gauze Pads
- Bandages
- Butterfly needles and hubs
- Microcentrifuge tube rack
- Test tube rack
- Sharps bin and lid

In order to process samples consistently across all projects and ensure the highest quality samples possible, project sites must have access to the following equipment:

- Centrifuge capable of  $\geq 1500$  rcf (1500 x g) with refrigeration to 4°C
- -80°C Freezer

In order to ship specimens, you must provide:

- Dry ice (minimum 10 pounds per shipment)

## 6.0 SPECIMEN LABELS

Labels must be affixed on all collection and aliquot tubes to ensure unique specimen identity. BioSEND provides labels for all samples being collected and returned to BioSEND. The site is responsible for providing labels for biospecimens that will be retained at the site. If labels are provided but the sample is not collected, please discard the unused labels.

### 6.1 Types of Labels

Each kit contains all labels required for the return of biospecimens to BioSEND.



The **Kit Labels** do not indicate a specimen type, but are affixed on BioSEND forms and on specific packing materials. See Appendix K for further instructions.




The **Specimen Labels** are placed on specimen tubes shipped to BioSEND. Each Specimen Label has a unique barcode that is tied to the Kit. The specimen type and collection tube will be noted on the tube. For example, the label to the left would be placed on a plasma aliquot generated from a 10ml EDTA tube.

## 6.2 Affixing Labels

In order to ensure the label adheres properly and remains on the tube, follow these instructions:

- Place specimen labels on **ALL** collection tubes and cryovials **BEFORE** sample collection, sample processing, or freezing. This will help to ensure the label properly adheres to the tube before exposure to moisture or different temperatures.
- The blood collection tube labels contain a 2D barcode on the left hand side of the label. When turned horizontally, the barcode should be closer to the top (cap end) of the tube.
- Place label **horizontally** on the tube (wrapped around sideways if the tube is upright); see below.

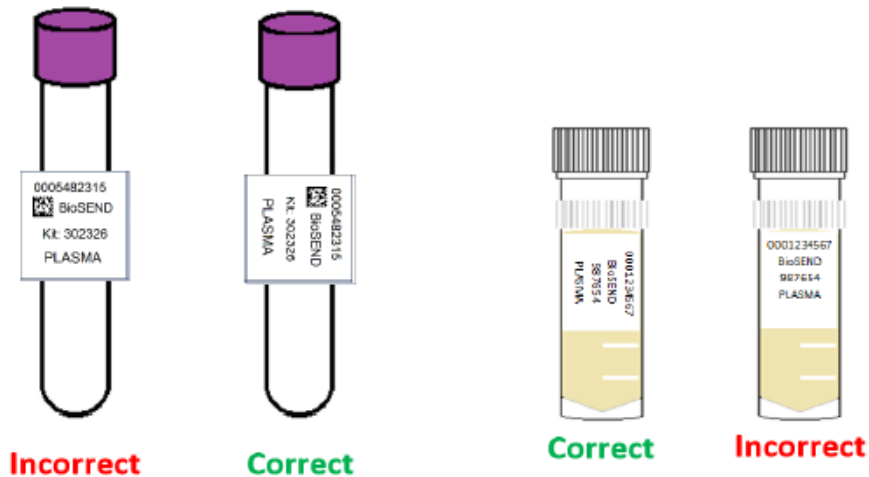

- Take a moment to ensure the label is **completely affixed** to each tube. It may be helpful to roll the tube between your fingers after applying the label.

## **7.0 SPECIMEN COLLECTION AND PROCESSING PROCEDURES**

Consistency in sample collection and processing is essential for biomarker studies. All samples are drawn in the same order and then processed in a uniform fashion. **Please read the instructions before collecting any specimens. Have all your supplies and equipment out and prepared prior to drawing blood.**


### **7.1 Blood Collection Protocols**

- Appendix B: Whole Blood Collection for Isolation of Plasma and Buffy Coat
- Appendix D: Whole Blood Collection (No Processing)
- Appendix F: Whole Blood Collection for the Isolation of Serum

**PBMCs will be isolated at Johns Hopkins in the Calabresi Lab per their internal protocol. The Calabresi lab will process enough blood sample to isolate an additional  $6 \times 10^6$  cells, to be shipped to BioSEND in 2 aliquots.**

#### 7.4 Filling Aliquot Tubes (Plasma and Serum)

In order to ensure that BioSEND receives a sufficient amount of sample for processing and storage, and to avoid cracking of the tubes prior to shipment, each aliquot tube should be filled to the assigned volume (refer to detailed processing instructions for average yield per sample). Over-filled tubes may burst once placed in the freezer, resulting in a loss of that sample. Each site is supplied with sufficient collection tubes to provide the specimen volume described in the Protocol Schedules for Biospecimen Submission ([see Section 4](#)). Specimens collected in addition to those described in Section 4 are collected at the site's discretion and are not returned to BioSEND.

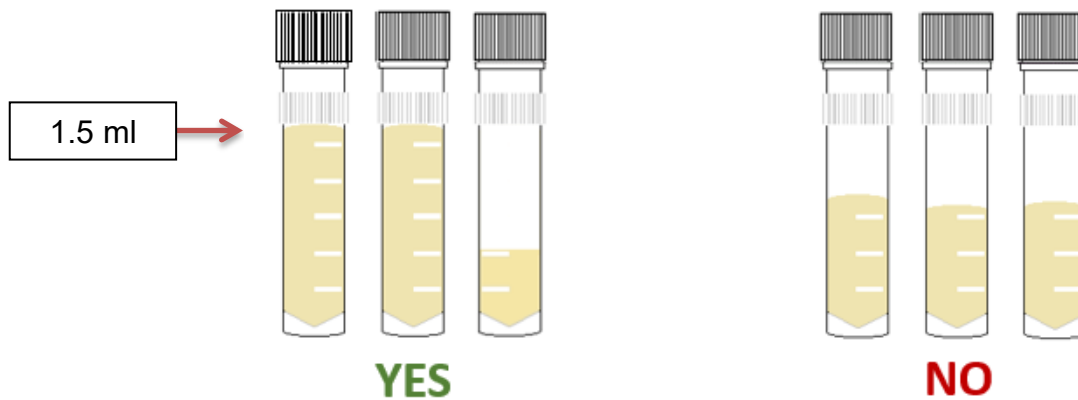

## **8.0 Packaging and Shipping Instructions**

**ALL** study personnel responsible for shipping should be certified in biospecimen shipping. If not available at your institution, training and certification is available through the CITI training site (Course titled “Shipping and Transport of Regulated Biological Materials” at <https://www.citiprogram.org/>).

We encourage all studies to use our custom UPS shipping interface to create shipping waybills and schedule package pickups. More information can be found at <https://biosend.org/shipping-resources>.

### **8.1 Specimen Collection and Processing Form**

The Specimen Collection and Processing Form should be completed for all samples submitted to BioSEND. Please see Appendix I for further instructions.

### **8.2 Shipping Instructions**

Please reference Appendix K for frozen shipping instructions and Appendix Q for generating airway bills and scheduling pick-ups.



### **8.3 Shipping Address**

All samples are shipped to the BioSEND laboratory:

BioSEND  
Indiana University School of Medicine  
351 W. 10<sup>th</sup> Street. TK-217  
Indianapolis, IN 46202-5188

## 9.0 Reconciliation and Non-Conformance

Appendix I must be completed the day that samples are collected to capture information related to sample collection and processing. This form includes information that will be used to reconcile sample collection and receipt, as well as information essential to future analyses.

BioSEND will contact the site as soon as possible when a discrepancy or issue is found with either the samples or paperwork.

Common non-conformance issues that will result in BioSEND staff contacting your site include:

- Missing samples (samples documented on the sample form that are not physically present in the shipment)
- Incorrect samples collected and shipped
- Damaged or incorrectly prepared samples
- Unlabeled or mislabeled samples
- Samples frozen and stored longer than three months at the site

## **10.0 APPENDICES**

Appendix B: Whole Blood Collection for Isolation of Plasma and Buffy Coat

Appendix D: Whole Blood Collection (No Processing)

Appendix F: Whole Blood Collection for the Isolation of Serum

Appendix I: Specimen Collection and Processing Form

Appendix K: Frozen Shipping Instructions

Appendix Q: UPS ShipExec™ Thin Client Instructions

## Appendix B – Whole Blood Collection for Plasma and Buffy Coat

Whole Blood Collection for Plasma and Buffy Coat using 10 ml EDTA (glass) tube

1. Store empty EDTA (glass) tubes at room temperature 64°F – 77°F (18°C to 25°C) prior to use.
2. Place “PLASMA” specimen labels on the 10 ml EDTA tube and on the three purple-capped 2 ml cryovial tubes. Place “BUFFY COAT” specimen labels on the a clear-capped 2ml cryovial tubes.
3. Pre-chill the labeled cryovials on wet ice for at least 5 minutes.
4. Set centrifuge to 4°C to pre-chill before use. Time needed to pre-chill the centrifuge to 4°C will depend on your centrifuge model.
5. Collect whole blood into the tubes using your institution’s recommended procedure for standard venipuncture technique.
  - a. Subject is required to lay down for 30 minutes after IV catheter is placed before the blood draw occurs.
  - b. Collect blood directly from the IV catheter using a Luer adapter.
6. Allow at least 10 seconds for a complete blood draw to take place in each tube. Ensure that the blood has stopped flowing into the tube before removing the tube from the holder. The tube vacuum is designed to draw 10 ml of blood into the tube.
7. Immediately after blood collection, gently invert/mix (180 degree turns) the EDTA tube 8 – 10 times. **Do not shake the tubes!**
8. Within 30 minutes of blood collection, centrifuge balanced tubes for 15 minutes at 1500 RCF (x g) at 4°C. It is critical that the tubes be centrifuged at the appropriate speed and temperature to ensure proper plasma separation.
9. Remove the plasma by tilting the tube and placing the pipette tip along the lower side of the wall. **Use caution not to touch the buffy coat or packed red blood cells at the bottom of the**


**tube so that the plasma is not contaminated** (see below). Using a disposable tipped micropipette, transfer plasma into the purple-capped cryovials. Aliquot 1.5 ml per cryovial. If you cannot obtain 3 plasma aliquots, please note “low volume draw” on the Sample Record and Shipment Notification form (Appendix I) under “Notification of Problems”. Each 10 ml EDTA tube should yield approximately 4-5 ml of plasma.

10. After plasma has been removed from the EDTA tubes, aliquot buffy coat layer (see figure below) into clear-capped cryovial using a disposable graduated micropipette. All of the buffy coat from a single 10 ml EDTA tube will be placed into one cryovial. The buffy coat aliquot is expected to have a reddish color from the red blood cells.



11. After plasma and buffy coat has been aliquoted into cryovials, **discard** the 10ml EDTA collection tube. Do not send these tubes to BioSEND.
12. Complete the Sample Record and Shipment Notification form (Appendix I).
13. Place the labeled cryovials in the 25 slot cryobox. Place the cryobox UPRIGHT on dry ice. Transfer to **-80°C freezer as soon as possible, within 2 hours of blood draw**. Store all samples at -80°C until shipped to BioSEND on dry ice.
14. Ship the frozen plasma aliquots to BioSEND according to Appendix K – Frozen Shipping Instructions.

## Plasma and Buffy Coat Collection and Preparation – 10ml K3 EDTA (glass) Tube

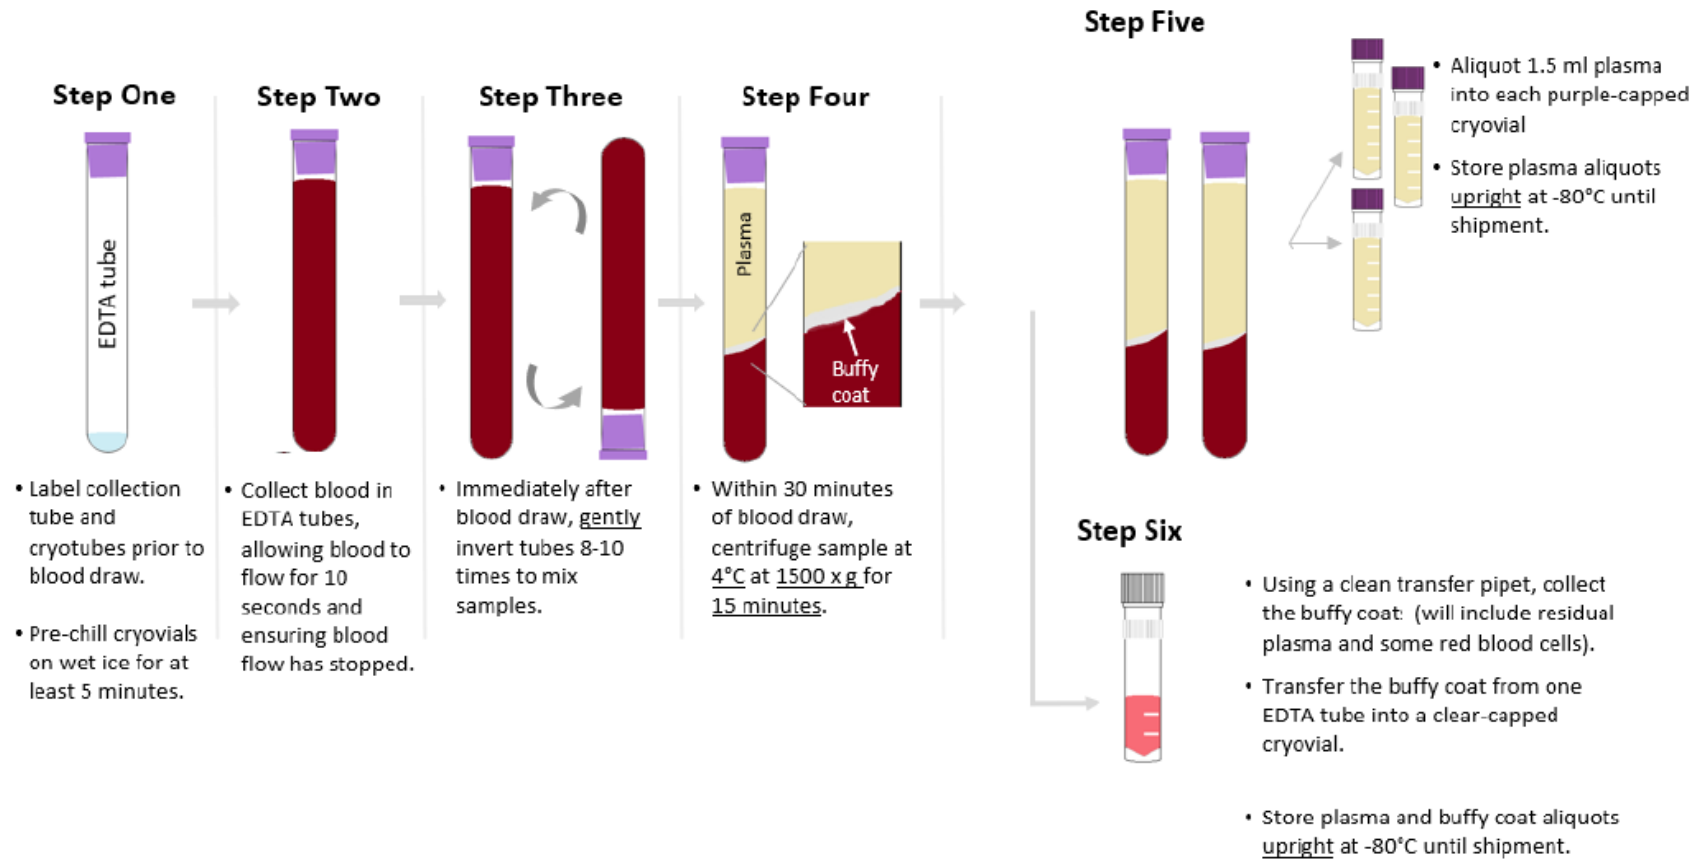

## Appendix D – Whole Blood Collection (No Processing)


One 3ml Purple-Top EDTA Tube is provided by BioSEND for Whole Blood collection (to be shipped to BioSEND FROZEN; no processing required).

1. Store empty tubes and collection supplies at room temperature, 64°F - 77°F (18°C to 25°C) before use.
2. Place pre-printed specimen label (WBLD) on the **one 3ml purple top EDTA tube** prior to blood draw.
3. Using a blood collection set and a holder, collect whole blood into the tubes using your institution's recommended procedure for standard venipuncture technique.

*The following techniques shall be used to prevent possible backflow:*

- a. Place donor's arm in a downward position.
  - b. Hold tube in a vertical position, below the donor's arm during blood collection.
  - c. Release tourniquet as soon as blood starts to flow into tube.
  - d. Make sure tube additives do not touch stopper or end of the needle during venipuncture.
4. **Immediately after blood collection, gently invert/mix (180 degree turns) the EDTA tube 8-10 times. Do not shake the tube!**
  5. Complete the Sample Record and Shipment Notification form (Appendix I).
  6. Place the Purple-Top EDTA in a **WIRE** or **PLASTIC** rack. Do **NOT** use a Styrofoam rack. This will cause the Purple-Top EDTA tube to crack when frozen. Place the Purple-Top EDTA tube immediately to a **-80°C Freezer**.
  7. Ship the whole blood tube to BioSEND according to **Appendix K - Frozen Shipping Instructions**.

## WBLD Preparation – 1 x 3 ml K2 EDTA (Purple Top) Tube

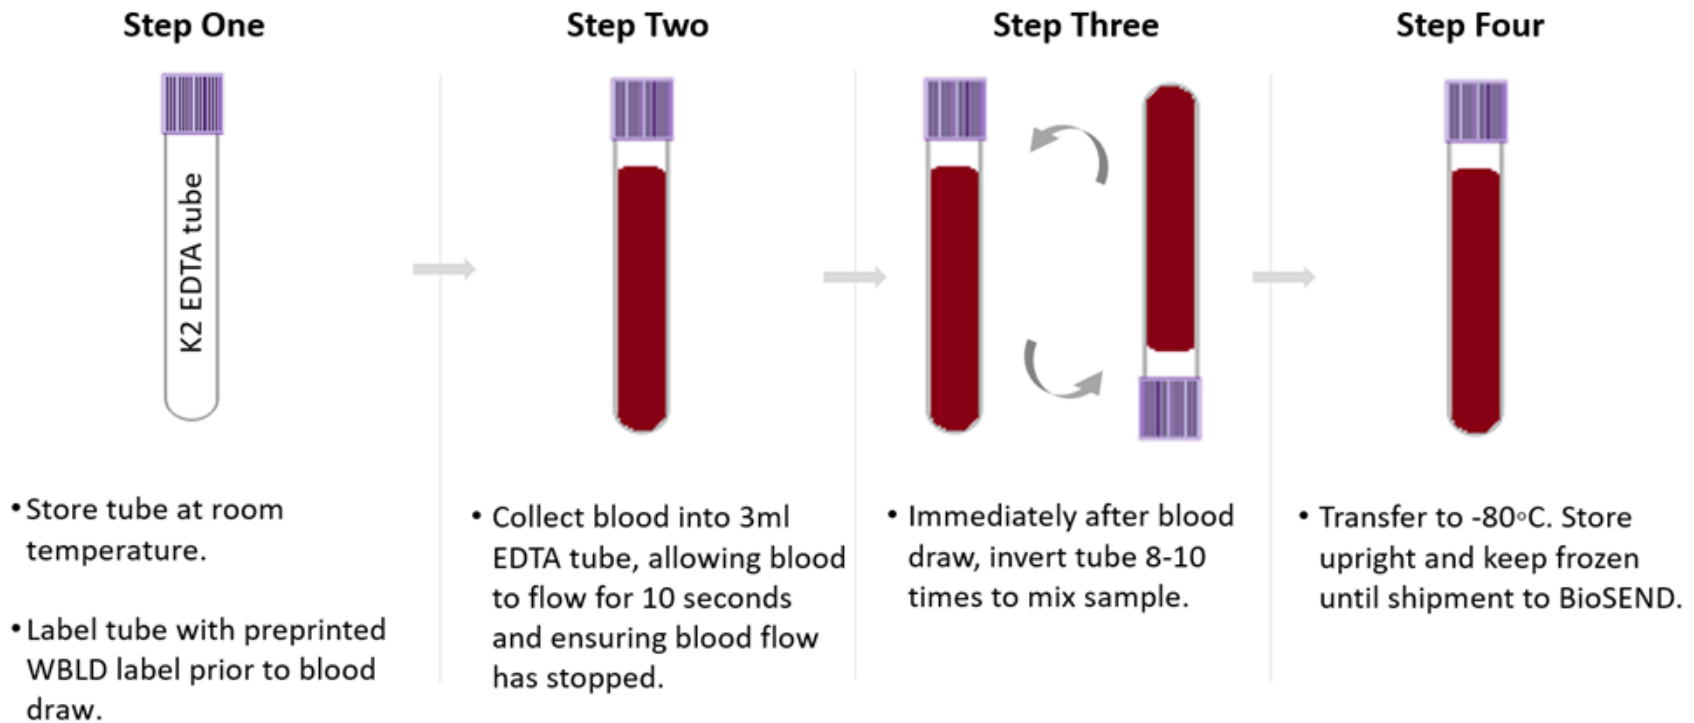



## Appendix F – Whole Blood Collection for Isolation of Serum

**Whole Blood Collection for Isolation of Serum: 10 ml red-top serum (glass) tube and cryovials are provided by BioSEND for the collection of serum.**


1. Store empty serum determination (red-top) tubes at room temperature 64°F – 77°F (18°C to 25°C) prior to use.
2. Place pre-printed specimen labels noted as “SERUM” on the serum determination red-top tube and on three of the 2 ml cryovials prior to blood draw. Three cryovials will be shipped to BioSEND; the remaining cryovials will be retained by the site and labeled accordingly.
3. Pre-chill labeled cryovials on wet ice for at least 5 minutes or longer.
4. Set centrifuge to 4°C to pre-chill before use. Time needed to pre-chill the centrifuge to 4°C will depend on your centrifuge model.
5. Collect whole blood into the tubes using your institution’s recommended procedure for standard venipuncture technique.
  - a. Subject is required to lay down for 30 minutes after IV catheter is placed before the blood draw occurs.
  - b. Collect blood directly from the IV catheter using a Luer adapter.
6. Allow at least 10 seconds for a complete blood draw to take place in each tube. Ensure that the blood has stopped flowing into the tube before removing the tube from the holder. The tube with its vacuum is designed to draw 10 ml of blood into the tube.
7. Immediately after blood collection, **gently** invert/mix (180 degree turns) the serum determination tube 8-10 times. **Do not shake the tubes!**
8. Allow blood to clot at room temperature for **at least 30 minutes**.
  - ❖ Within 30 to 60 minutes from blood collection, centrifuge balanced tubes for 15 minutes at 1500 RCF (x g) at 4°C. It is critical that the tubes be centrifuged at the appropriate speed and temperature to ensure proper serum separation.

9. Remove the serum by tilting the tube and placing the pipette tip along the lower side of the tube wall. Use caution to pipet only the serum layer and not the red blood cell layer. Using a disposable tipped micropipette, transfer serum into the pre-labeled cryovials. Aliquot 1.5 ml per cryovial. Send 3 x 1.5 ml aliquots to BioSEND.


10. Complete the Sample Record and Shipment Notification form (Appendix I).

11. Place the labeled cryovials in the 25 slot cryovial box. Transfer to -80°C Freezer as soon as possible, **ensuring cryovials are frozen upright**. Store all samples upright at -80°C until shipped to BioSEND on dry ice.

12. Ship the frozen serum aliquots to BioSEND according to Appendix K – Frozen Shipping Instructions.

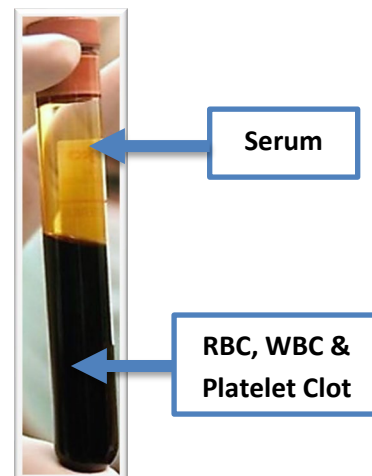

## Serum Preparation –10 ml Serum (Red Top) Tube

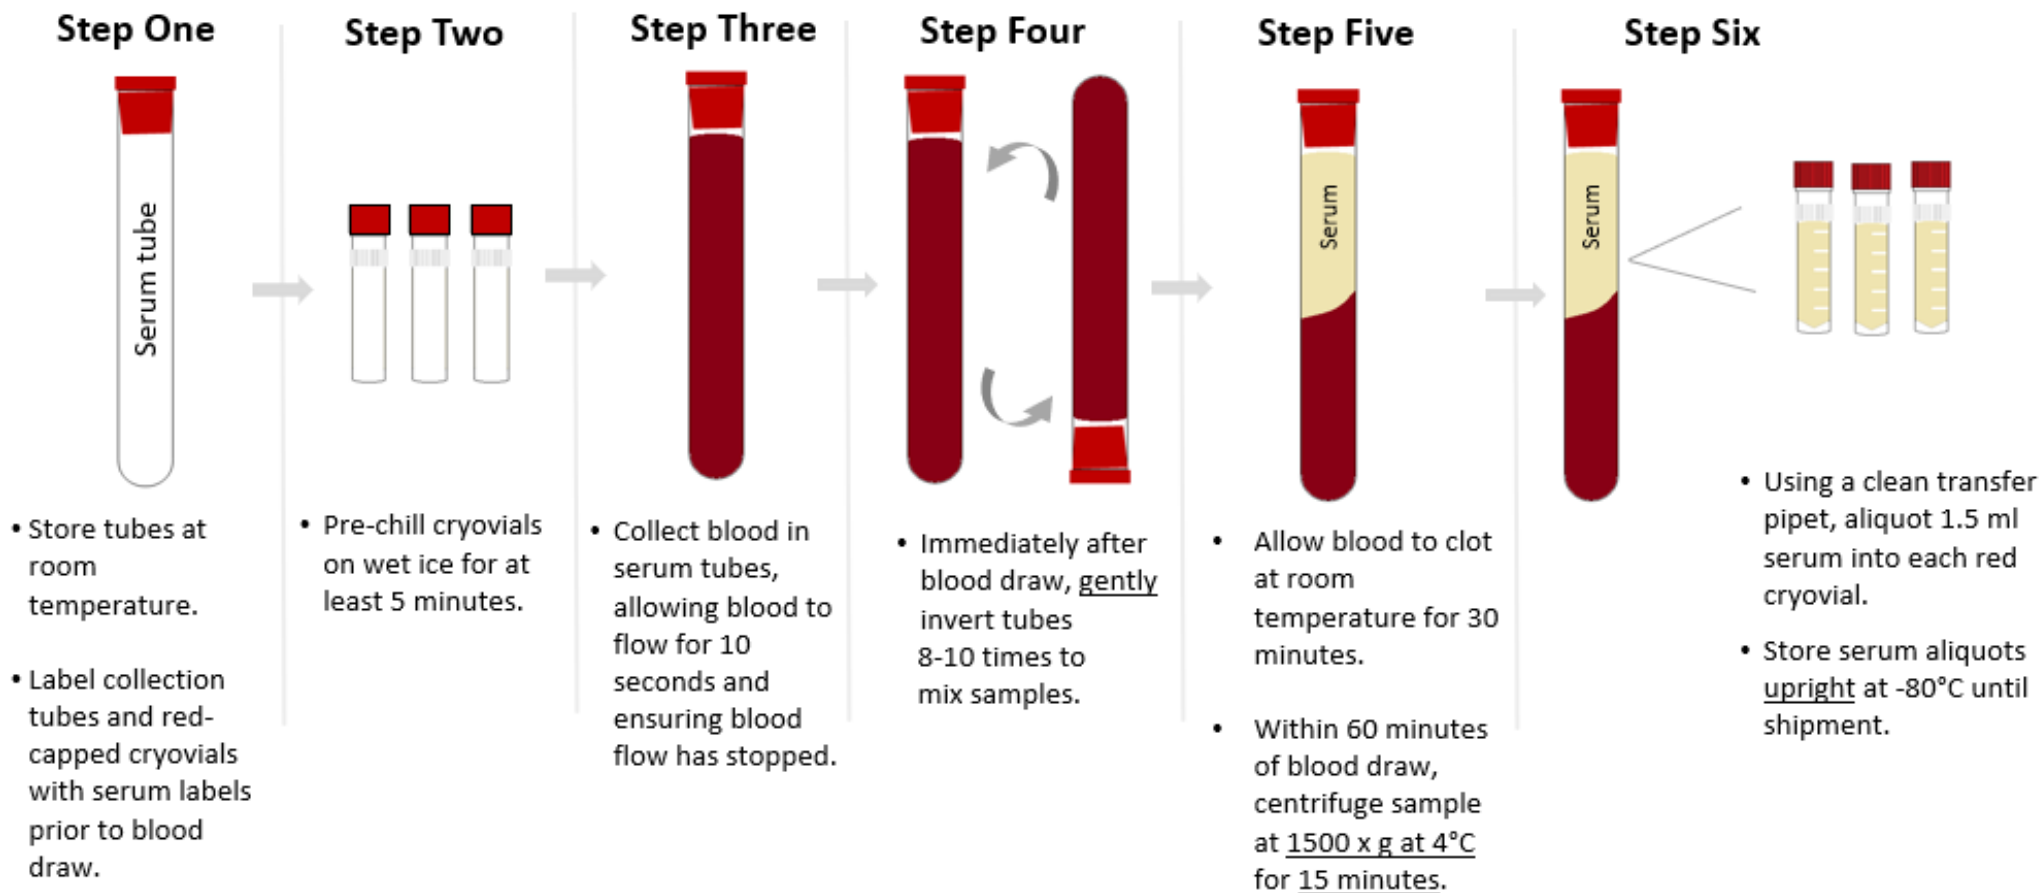

## Appendix I – Sample Collection and Processing Form

A Sample Collection and Processing Form must be completed for each subject-visit submitted to BioSEND. This form includes a Frozen Shipping Manifest that should be completed in advance of shipping to BioSEND. A copy of this form should also be included in the shipper. A copy of the form will be emailed to you upon completion. The form can be completed via REDCap by following the bellow link:

- **Link to Sample Collection and Processing Form:** <https://redcap.link/MICRO-PDSampleForm>

Please note that there is a Save & Return option at the bottom of the survey. This may be used if, for example, you are ready to complete the Collection and Processing portion of the form, but not yet ready to complete the Frozen Shipping Manifest.

Clicking “Submit” at the end of the Frozen Shipping Manifest portion of the form will send an automatic notification to BioSEND of your shipment.

If unable to access REDCap during collection and processing, the form on the following may be printed and completed by hand. If your site has a separate processing lab from your coordinating team, you can share this form with them so that they may capture and return this data to you. This form is provided to aid with processing data collection. Data must be entered into REDCap when site staff is able to do so.

For links to your sample processing form, to download the most recent version of of this manual, and access recordings of BioSEND trainings, please visit <https://biosend.org/coordinate-studies/active-studies> and choose your study from the drop-down list.

# MICRO-PD Specimen Collection And Processing Form

Protocol: MICRO-PD

Please complete the Specimen Collection and Processing Form, below.

---

Study Site  Johns Hopkins University

---

Email address of staff member completing this form \_\_\_\_\_

Note: A copy of the completed sample form and the shipping manifest will be sent to this address.

---

GUID: \_\_\_\_\_

---

Sex (used for DNA quality control)  Male  
 Female  
 Other

---

Visit  BL

---

IU Kit Number \_\_\_\_\_

**Blood Collection and Processing**

Date of venipuncture blood collection

---

Time of venipuncture blood collection

---

  
(Use 24 Hour clock)

Date participant last ate

---

Time participant last ate

---

1. SERUM (red-top tube, 10 mL)

Was blood collected and processed for SERUM?

- Yes  
 No

Blood volume collected for SERUM

---

  
(mL)

Reason volume collected for serum was less than standard

- Difficult stick/poor veins  
 Patient dehydrated  
 Bad tube vacuum  
 Other  
(mL)

Time of SERUM tube centrifugation

---

  
(Use 24 Hour clock)

Duration of SERUM tube centrifugation

---

  
(minutes)

Rate of SERUM tube centrifugation

---

  
(x g)

Temperature of SERUM tube centrifugation

---

  
(degrees Celsius)

Number of SERUM aliquots created for BioSEND

---

  
(Each aliquot should be 1.5 mL)

Date SERUM aliquots were placed in freezer

---

Time SERUM aliquots were placed in freezer

---

  
(Use 24 Hour clock.)

---

SERUM storage temperature

\_\_\_\_\_  
(degrees Celsius)

---

SERUM notes

\_\_\_\_\_

---

2. PLASMA and BUFFY COAT (Purple-top EDTA tube, 10 mL)

Was blood collected and processed for PLASMA EDTA?

- Yes  
 No
- 

Blood volume collected for PLASMA EDTA

\_\_\_\_\_  
(mL)

---

Reason volume collected for plasma was less than standard

- Difficult stick/poor veins  
 Patient dehydrated  
 Bad tube vacuum  
 Other  
(mL)
- 

Time of PLASMA EDTA tube centrifugation

\_\_\_\_\_  
(Use 24 Hour clock)

---

Duration of PLASMA EDTA tube centrifugation

\_\_\_\_\_  
(minutes)

---

Rate of PLASMA EDTA tube centrifugation

\_\_\_\_\_  
(x g)

---

Temperature of PLASMA EDTA tube centrifugation

\_\_\_\_\_  
(degrees Celsius)

---

Number of PLASMA EDTA aliquots created for BioSEND

\_\_\_\_\_  
(Each aliquot should be 1.5 mL)

---

Number of BUFFY COAT aliquots created for BioSEND

\_\_\_\_\_

---

Date PLASMA EDTA and BUFFY COAT were placed in freezer

\_\_\_\_\_

---

Time PLASMA EDTA and BUFFY COAT were placed in freezer

\_\_\_\_\_  
(Use 24 Hour clock.)

---

PLASMA EDTA and BUFFY COAT storage temperature

\_\_\_\_\_  
(degrees Celsius)

---

---

PLASMA EDTA notes

---

---

3. WHOLE BLOOD (EDTA tube, 3 mL)

---

Was blood collected for WBLD?

- Yes
  - No
- 

Number of WBLD tubes collected

\_\_\_\_\_ (One 3ml EDTA tube expected)

---

Date WBLD was placed in freezer

\_\_\_\_\_

---

Time WBLD was placed in freezer

\_\_\_\_\_ (Use 24 Hour clock)

---

WBLD storage temperature

\_\_\_\_\_ (degrees Celsius)

---

WBLD notes

---

---

4. PBMC (NaHep tube, 10 mL)

---

Was blood collected for PBMC?

- Yes
  - No
- 

Number of PBMC aliquots created for BioSEND

\_\_\_\_\_ (Two 5ml aliquots expected)

---

Date PBMC aliquots were placed in freezer

\_\_\_\_\_

---

Time PBMC was placed in freezer

\_\_\_\_\_ (Use 24 Hour clock)

---

PBMC storage temperature

\_\_\_\_\_ (degrees Celsius)

---

PBMC notes

---



# MICRO-PD Frozen Shipping Manifest

Please verify/update the information below. When you click the "Submit" button below, a PDF copy of the Frozen Shipping Manifest will be emailed to you for Subject [subj\_id].

Please print a copy of that document and include it in the Kit #[kit\_num] shipping container.

Study \_\_\_\_\_

Study Site: \_\_\_\_\_

GUID: \_\_\_\_\_

Visit: \_\_\_\_\_

IU Kit Number: \_\_\_\_\_

Date of blood collection: \_\_\_\_\_

## SERUM

Number of SERUM aliquots shipped: \_\_\_\_\_

## PLASMA EDTA

Number of PLASMA EDTA aliquots shipped: \_\_\_\_\_

Number of BUFFY COAT aliquots shipped: \_\_\_\_\_

## WHOLE BLOOD EDTA

Number of WHOLE BLOOD tubes shipped: \_\_\_\_\_

## PBMC

Number of PBMC aliquots shipped: \_\_\_\_\_

**Shipping Information - Please complete.**

Frozen shipments should be sent Monday-Wednesday only. Please check for holiday closures prior to shipping. Contact us at biosend@iu.edu if you are unsure whether or not it is safe to ship.

Date of shipment:

---

Did/will you use the IU UPS interface to generate the shipping label?

- Yes  
 No

Which shipping service did you use?

- UPS  
 FedEx  
 World Courier  
 Other

What is the shipment tracking number?

---

## Appendix K – Frozen Shipping Instructions

### IMPORTANT!

Frozen samples must be shipped Monday – Wednesday only,  
using Next Day Air delivery

Please be aware of holidays and inclement weather and plan your shipments accordingly. Reach out to [biosend@iu.edu](mailto:biosend@iu.edu) if you have any questions

Specimens being shipped to BioSEND are Category B UN3373 specimens and as such must be triple packaged and compliant with IATA Packing Instructions. *See the latest eEdition of the IATA regulations for complete documentation.*

Triple packaging consists of a primary receptacle(s), a secondary packaging, and a rigid outer packaging. The primary receptacles must be packed in secondary packaging in such a way that, under normal conditions of transport, they cannot break, be punctured, or leak their contents into the secondary packaging. Secondary packaging must be secured in outer packaging with suitable cushioning material. Any leakage of the contents must not compromise the integrity of the cushioning material or of the outer packaging.

### IATA Packing and Labeling Guidelines

- The primary receptacle (cryovials or blood collection tubes) must be leak proof and must not contain more than 1 L total.
- The secondary packaging (plastic canister or biohazard bag) must be leak proof and if multiple blood tubes are placed in a single secondary packaging, they must be either individually wrapped or separated to prevent direct contact with adjacent blood tubes.
- Absorbent material must be placed between the primary receptacle (cryovials or blood collection tubes) and the secondary packaging. The absorbent material must be of sufficient quantity to absorb the entire contents of the specimens being shipped. Examples of absorbent material are paper towels, absorbent pads, cotton balls, or cellulose wadding.
- A shipping manifest listing the specimens being shipped must be included between the secondary and outer packaging.
- The outer shipping container must display the following labels:
  - ✓ Sender's name and address
  - ✓ Recipient's name and address
  - ✓ Responsible persons (shipper and recipient)
  - ✓ The words "Biological Substance, Category B"
  - ✓ UN3373
  - ✓ Class 9 label including UN 1845, and net weight of dry ice contained

## BioSEND Packaging and Shipment Instructions – Frozen Shipments


1. Generate airway bill and schedule courier pick-up, as needed.
  - For instructions on generating airway bills and scheduling using the UPS ShipExec™ Thin Client system, see Appendix Q.
2. Record the tracking number onto the Sample Record and Shipment Notification form (Appendix I).
3. Make a copy of the Sample Record and Shipment Notification form.
4. Place all frozen labeled cryotubes in the cryobox. Only include specimens from one subject in each cryobox.
5. Place the cryobox in a clear plastic biohazard bag (do NOT remove the absorbent material found in the bag), and seal the biohazard bag according to the instructions on the bag. Affix a kit label to the outside of the biohazard bag.



6. Place approximately 2-3 inches of dry ice in the bottom of the Styrofoam® shipping container.
7. If your protocol is collecting frozen whole blood, DNA, or RNA, place labeled tubes in bubble sleeves and seal.
8. Place the tubes in a clear plastic biohazard bag (do NOT remove the absorbent material found in the bag), and seal the biohazard bag according to the instructions on the bag. Affix a Case Label to the outside of the biohazard bag.
9. Place the biohazard bag containing the cryobox into the provided Styrofoam® shipping container on top of the dry ice. Please ensure that the cryobox is placed so that the cryovials are upright in the shipping container (as pictured).



10. Fully cover the cryobox with approximately 2 inches of dry ice. Do not include more than 2 subjects' worth of samples in a single shipper.
11. If including additional biohazard bags in package, include a layer of dry ice (approximately 2 inches) between each biohazard bag.
12. The inner Styrofoam® shipping container must contain a minimum of 10 lbs (or 4.5 kg) of dry ice. The dry ice should entirely fill the inner box to ensure the frozen state of the specimens.
13. Replace the lid on the Styrofoam® container. Place the completed Sample Record and Shipment Notification form in the package on top of the Styrofoam® lid for each patient specimen, and close and seal the outer cardboard shipping carton with packing tape.
14. Print a copy of your UPS® airway bill generated through the UPS ShipExec™ Thin Client system (see Appendix Q). Place airway bill into the provided airway bill envelope and affix envelope to package.
15. Complete the UPS Dry Ice Label with the following information:
  - Net weight of dry ice in kg (this amount must match the amount recorded on the airway bill)

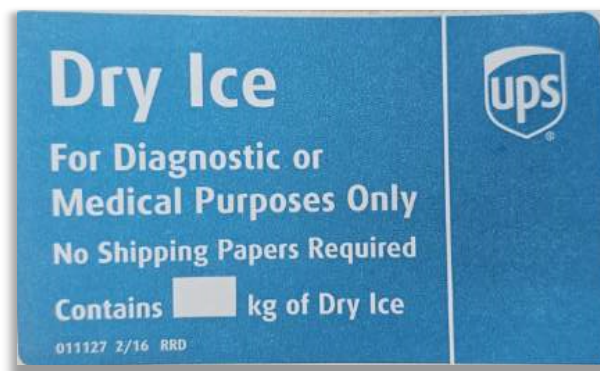

- Do not cover any part of this label with other stickers, including pre-printed address labels.

<b>IMPORTANT!</b>
Complete the required fields on your airway bill and Class 9 Dry Ice labels, or courier may reject or return your package.

16. Apply all provided warning labels (UN3373, Dry Ice Label and Fragile Label), taking care not to overlap labels with each other or with airway bill.
17. Hold packaged samples in -80°C freezer until time of courier pick-up/drop-off.
18. Specimens should be sent to the address below. Frozen shipments should be sent Monday through Wednesday only to avoid shipping delays on Thursday or Friday.

BioSEND  
IU School of Medicine  
351 W. 10<sup>th</sup> Street  
TK-217  
Indianapolis, IN 46202

19. **Notify BioSEND of your shipment by completing the Specimen Collection and Processing Form and Frozen Shipping Manifest in REDCap (see Appendix I for details). Submission of this form will send an automatic notification of your shipment to the BioSEND team.**
20. Use courier tracking system to ensure the delivery occurs as scheduled and is received by BioSEND.

In addition to tracking and reconciliation of samples, the condition and amount of samples received are tracked by BioSEND for each sample type. Investigators and clinical coordinators for each project are responsible for ensuring that the requested amounts of each fluid are collected to the best of their ability and that samples are packed with sufficient amounts of dry ice to avoid thawing in the shipment process.

## Appendix Q - UPS ShipExec™ Thin Client Instructions

**\*\*\* The shipment label in ShipExec should not be created until the day of shipment \*\*\***

- 1) Log in to the UPS ShipExec™ Thin Client website: <https://kits.iu.edu/UPS> or <https://kits.iu.edu/ups>.
  - a. To request an account, complete the following survey: <https://redcap.uits.iu.edu/surveys/?s=88TTWY3KAF>
- 2) Find the “Shipping” dropdown menu in the top left corner of the screen and click on “Shipping and Rating”.
- 3) Once the Indiana University page loads, look for the “Study Group” dropdown menu under “Shipment Information” on the right side of the screen. Choose your study from the dropdown menu.
- 4) After selecting your study, click on the magnifying glass icon on the left side of the screen under “Ship From”.
- 5) An address book and filters will populate the screen. On the right side of the screen, a list of all the site addresses within the study you selected should populate.
  - a. Filter the list down more by looking to the left side of the screen and searching for their address by filling in the “Company”, “Contact”, or “Address 1” fields. Click on the Search button when ready.
  - b. Once you have found your site address, click on the “Select” button to the left of the address.
- 6) Make sure your address populated in the fields under “Ship From” on the main page.
  - a. If you accidentally selected the wrong address, click on the “Reset” button on the bottom right of the screen. After the page reloads and clears the information, select your study again from the “Study Group” menu and click on the magnifying glass icon again to search for your correct address.
  - b. To change the address for your site and study group, please complete the following survey: <https://redcap.uits.iu.edu/surveys/?s=88TTWY3KAF>
- 7) Enter the total weight of your package in the “Weight” field on the right side of screen under the name of your study.
  - a. Leave the “Dry Ice Weight” field empty or enter “0” if shipping an ambient sample.
- 8) Enter the weight of the dry ice for frozen shipments in the “Dry Ice Weight” field.
  - a. The “Dry Ice Weight” field can *never* be higher than the “Weight” field.
  - b. **(Steps 9-10 can be skipped if you do not need to schedule a pickup)**
- 9) After entering the weights, click on the blue “Pickup Request” button.
- 10) When the Create Pickup Request box pops up, enter information into all the fields provided.
  - a. Enter the “Earliest Time Ready” and “Latest Time Ready” in 24-hour format.
    - i. Schedule pickup at a minimum 1 hour *before* the “Earliest Time Ready”
  - b. Choose a name and phone number that is the best contact if the UPS driver has question related to picking up your package
  - c. Entering the “Room Number” and “Floor” will help the UPS driver locate your package
    - i. The “Floor” field only allows numerical characters while the “Room Number” field is free text.
  - d. Click “Save” when done.
- 11) Once you are certain that all the correct information has been entered, click the “Ship” button in the bottom right corner of the screen.
- 12) If no red error messages pop up at the top of your screen after clicking on “Ship”, then you should have 2 downloaded PDF files: Shipment Receipt & UPS Package Label

- a. Shipment Receipt will list a “Pickup No.” that references your specific package if there is ever an issue with UPS picking up your package
- 13) Print out the UPS airway bill to any printer at your location.
- a. Fold the UPS airway bill and slide it inside the plastic UPS sleeve.
  - b. Peel the back off the plastic UPS sleeve and stick the sleeve to your package, making sure it is laying as flat as possible along the surface of the package.
- 14) Place your package in the spot designated in your pickup request, or wherever your daily UPS pickups occur.
- 15) If you need to reprint your airway bill or void your shipment, click on “History” at the top of the main screen.
- a. If your shipment does not automatically pop up, enter the date of shipment and then click “Search”.
  - b. To reprint your airway bill, click on the printer icon to the far left under “Action”
  - c. To void your shipment, click on the “X” icon to the far left under “Action”
    - i. If you created an airway bill that you no longer need, you must void the shipment to ensure your study will not be charged for the shipment.